

## NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: Dongguan HuaGang Communication Technology Co., Ltd.

Model Tested: KN95-A

Date Tested: June 22, 2020

These findings pertain to the Dongguan HuaGang Communication Technology Co., Ltd., model KN95-A. The packaging and labeling for this product indicate that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator) and EN149:2001+A1:2009 (the European standard for Respiratory Protective Devices – Filtering Half Masks to Protect Against Particles – Requirements, Testing, Marking).

Ten respirators were submitted for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found [here](#).

No certificate of approval was provided with the samples received; therefore, the authenticity of the claims cannot be validated.

The maximum and minimum filter efficiency was 98.79% and 98.05%, respectively. All ten respirators measured more than 95%.

While the above-listed product classification has similar performance requirements to NIOSH-approved devices, NIOSH does not have knowledge about the sustained manufacturer quality system and product quality control for these products. NIOSH also does not have knowledge about the product's handling and exposures after leaving its manufacturer's control.

In addition, this product is an ear loop design. Currently, there are no NIOSH-approved products with ear loops; NIOSH-approved N95s have head bands. Furthermore, limited assessment of ear loop designs, indicate difficulty achieving a proper fit. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

**This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process.** This assessment was developed as an assessment of the filter efficiency for those respirator's represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for [Crisis Capacity Strategies \(during known shortages\)](#).

## Evaluation of International Respirators

**Test:** Modified TEB-APR-STP-0059

**Date Tested:** June 22, 2020

**Report Prepared:** June 22, 2020

**Manufacturer:** Dongguan HuaGang Communication Technology Co., Ltd.

**Item Tested:** KN95-A

**Country of Certification:** China (GB2626-2006, EN149:2001+A1:2009)

Pictures have been added to the end of this report.


Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH <sub>2</sub> O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency
1	85	14.4	1.56	1.57	98.43
2	85	16.7	1.56	1.56	98.44
3	85	16.1	1.40	1.40	98.60
4	85	15.1	1.29	1.29	98.71
5	85	14.5	1.34	1.34	98.66
6	85	15.9	1.21	1.21	98.79
7	85	16.6	1.29	1.29	98.71
8	85	15.2	1.49	1.52	98.48
9	85	15.1	1.47	1.47	98.53
10	85	15.3	1.95	1.95	98.05
<b>Minimum Filter Efficiency: 98.05</b>			<b>Maximum Filter Efficiency: 98.79</b>		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment



# NPPTL COVID-19 Response: International Respirator Assessment

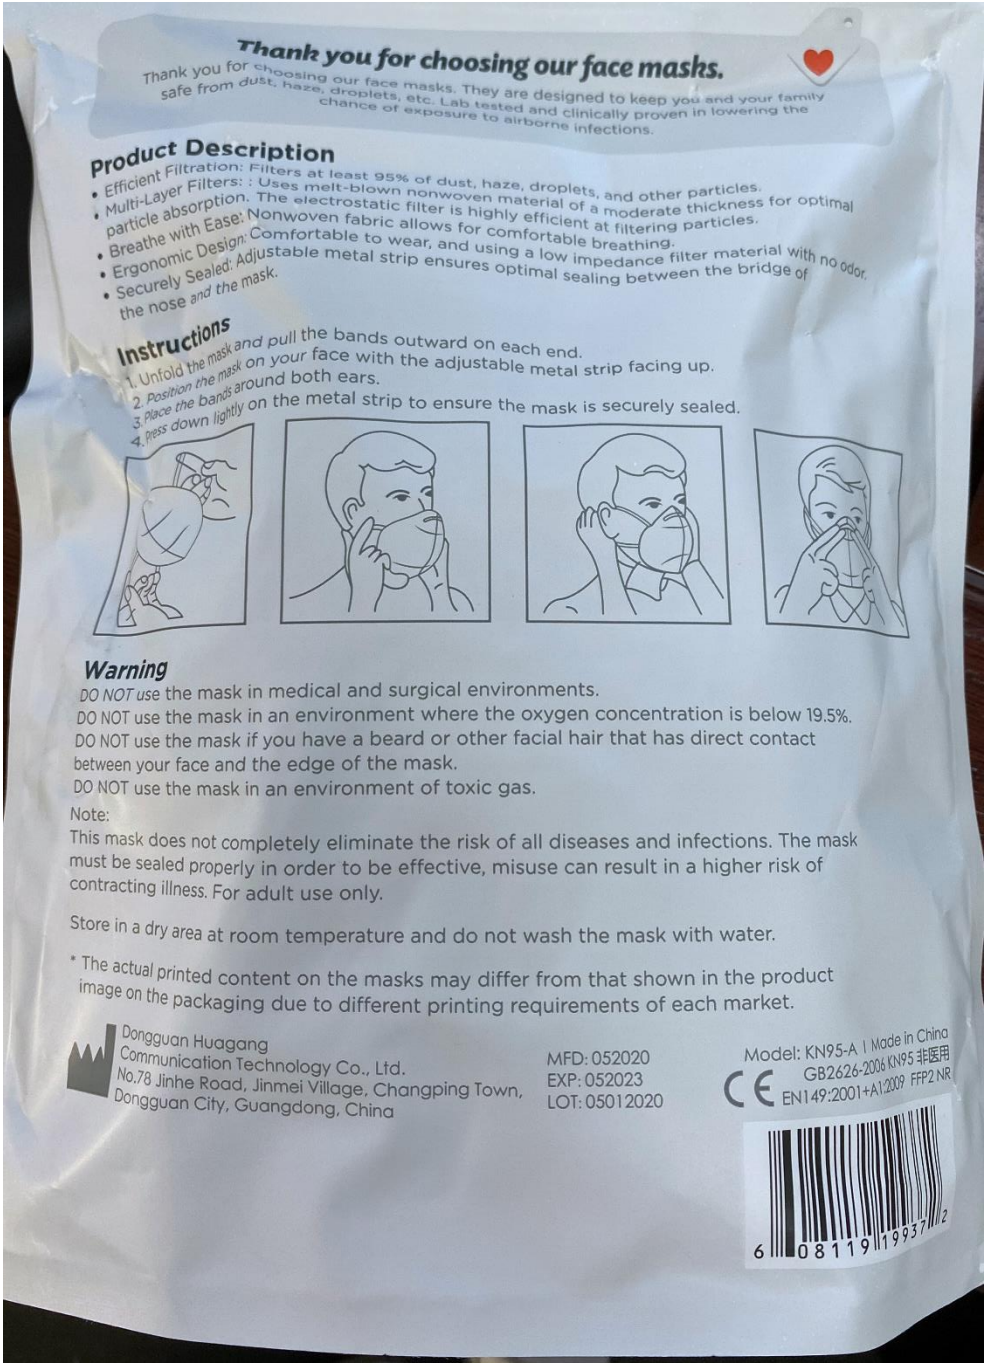

**Thank you for choosing our face masks.**  
Thank you for choosing our face masks. They are designed to keep you and your family safe from dust, haze, droplets, etc. Lab tested and clinically proven in lowering the chance of exposure to airborne infections.

### Product Description

- **Efficient Filtration:** Filters at least 95% of dust, haze, droplets, and other particles.
- **Multi-Layer Filters:** Uses melt-blown nonwoven material of a moderate thickness for optimal particle absorption. The electrostatic filter is highly efficient at filtering particles.
- **Breathe with Ease:** Nonwoven fabric allows for comfortable thickness for optimal breathing.
- **Ergonomic Design:** Comfortable to wear, and using a low impedance filter material with no odor.
- **Securely Sealed:** Adjustable metal strip ensures optimal sealing between the bridge of the nose and the mask.

### Instructions

1. Unfold the mask and pull the bands outward on each end.
2. Position the mask on your face with the adjustable metal strip facing up.
3. Place the bands around both ears.
4. Press down lightly on the metal strip to ensure the mask is securely sealed.



### Warning

- DO NOT use the mask in medical and surgical environments.
- DO NOT use the mask in an environment where the oxygen concentration is below 19.5%.
- DO NOT use the mask if you have a beard or other facial hair that has direct contact between your face and the edge of the mask.
- DO NOT use the mask in an environment of toxic gas.

**Note:**  
This mask does not completely eliminate the risk of all diseases and infections. The mask must be sealed properly in order to be effective, misuse can result in a higher risk of contracting illness. For adult use only.

Store in a dry area at room temperature and do not wash the mask with water.

\* The actual printed content on the masks may differ from that shown in the product image on the packaging due to different printing requirements of each market.

Dongguan Huagang  
Communication Technology Co., Ltd.  
No.78 Jinhe Road, Jinmei Village, Changping Town,  
Dongguan City, Guangdong, China

MFD: 052020  
EXP: 052023  
LOT: 05012020

Model: KN95-A | Made in China  
GB2626-2006 KN95 非医用  
EN149:2001+A1:2009 FFP2-NR



# 合格证

## QUALIFIED CERTIFICATE

<b>产品名称:</b> Product Name:	一次性防护口罩 (非医用) Disposable Face Mask (non-medical)
<b>型号(Model):</b>	KN95-A
<b>产品规格:</b> Specifications:	105 x 165mm (成人用) 105 x 165mm (for adult use)
<b>主要成分:</b> Main Material:	70%无纺布+30%熔喷布 70% non-woven fabric, 30% melt-blown fabric
<b>执行标准:</b> Executive Standard:	GB2626-2006 GB2626-2006
<b>生产日期:</b> Production Date:	052020 052020
<b>生产批次:</b> LOT:	05012020 05012020
<b>产品有效期:</b> Shelf Life:	3年 3 years
<b>存储条件:</b> Storage Instruction:	相对湿度不超过80%，避光干燥的室内环境下 Store in a clean, dry and ventilated environment. Relative humidity should not exceed 80%. Avoid direct sunlight.
<b>包装规格:</b> Packaging Specification:	见外包装 (See package)
<b>生产商:</b> Manufacturer:	东莞市华罡通讯科技有限公司 Dongguan Huagang Communication Technology Co., Ltd.
<b>生产地址:</b> Manufacturer Address:	广东省东莞市常平镇金美星河路二路78号 No.78 Jinhe Road, Jinmei Village, Changping Town, Dongguan City, Guangdong, China



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

